

Fiberscope for Safe and Secure Lacrimal Surgery

RUIDO Fiberscope allows observation of the whole lacrimal duct, which was impossible with the conventional devices.

Location and condition of the obstructive lesion can be examined before lacrimal probing.

Examination with RUIDO Fiberscope before and after lacrimal intubation improves effectiveness and safety of the operation.

Its inner channel enables direct irrigation of the lacrimal duct at the endoscopic surgery.

Lacrimal Ductoscope

RUIDO

RUIDO Fiberscope

Specifications

Type	Tip Shape	Outer Diameter (maximum)	Working Length	Channel Diameter	Overall Length	Field of View
MT3	Bent	0.7mm (1.0mm)	50mm	0.3mm	2,800mm	60°
MD10		0.9mm (1.2mm)				
MD6S	Straight	1.0mm (1.3mm)	70mm			


* EOG sterilizable

* Specifications are subject to change without notice.

■ Product Name : RUIDO Fiberscope

■ Regulatory Approval Number of Japan : 21400BZZ00022000


Images

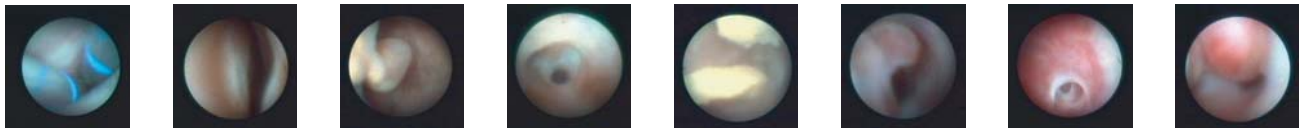


Photographed by Dr. T. Suzuki, Suzuki Eye Clinic

Shape of Insertion Portion

JP Patent No. 4124423

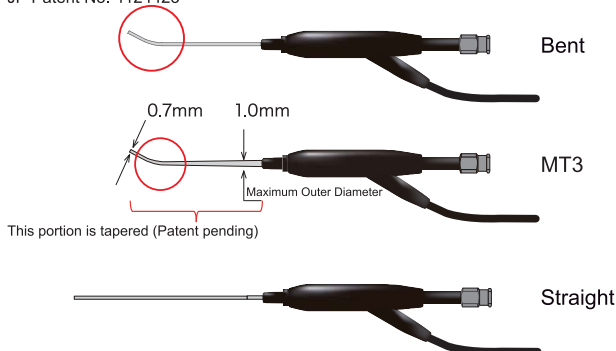

Components of Endoscope System

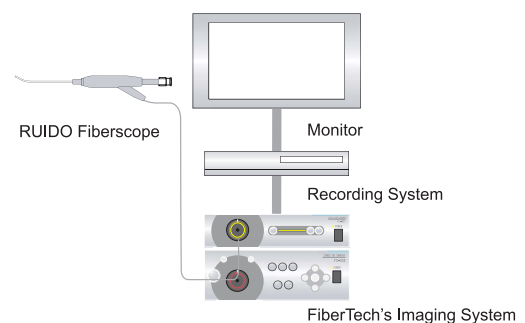

Manufactured by:

FiberTech Co., Ltd.

409-1 Nishimikado, Sakura City, Chiba 285-0074, Japan

Contact Information:

Phone: +81-3-5259-7600 FAX: +81-3-5259-1155

수입/판매원 : (주)성화메디칼

서울시 서초구 논현로 87, 삼호물산빌딩 B동 804호

Tel) 02-596-4380

Fax) 02-596-4383